Print on Plain White Paper (Part No. 122919)

Installation Instructions

Foot Control: 9A203001 9A233001

(1) Remove the foot control from the carton and inspect it for any shipping damage. If you detect damage, contact the shipping carrier and factory immediately.

(2) Before installing the foot control, review the operating procedures outlined in the table's Installation & Operation manual.

(3) Insert the coil cord of the foot control into either control port at the base of the table (see the illustration).

(4) The foot control is now ready for operation.

For additional information, refer to "Installing Optional Footswitch" within the Examination Table Installation and Operation Manual.

Clean the foot control periodically with a damp cloth and a mild soap solution. Always unplug the foot control coil cord from the table prior to cleaning and never immerse in water or other fluids.

If you have questions concerning the operation of your table or in the event of equipment failure, please contact your dealer. If you can't resolve your problem through your dealer, call Midmark at 1-800-MIDMARK.

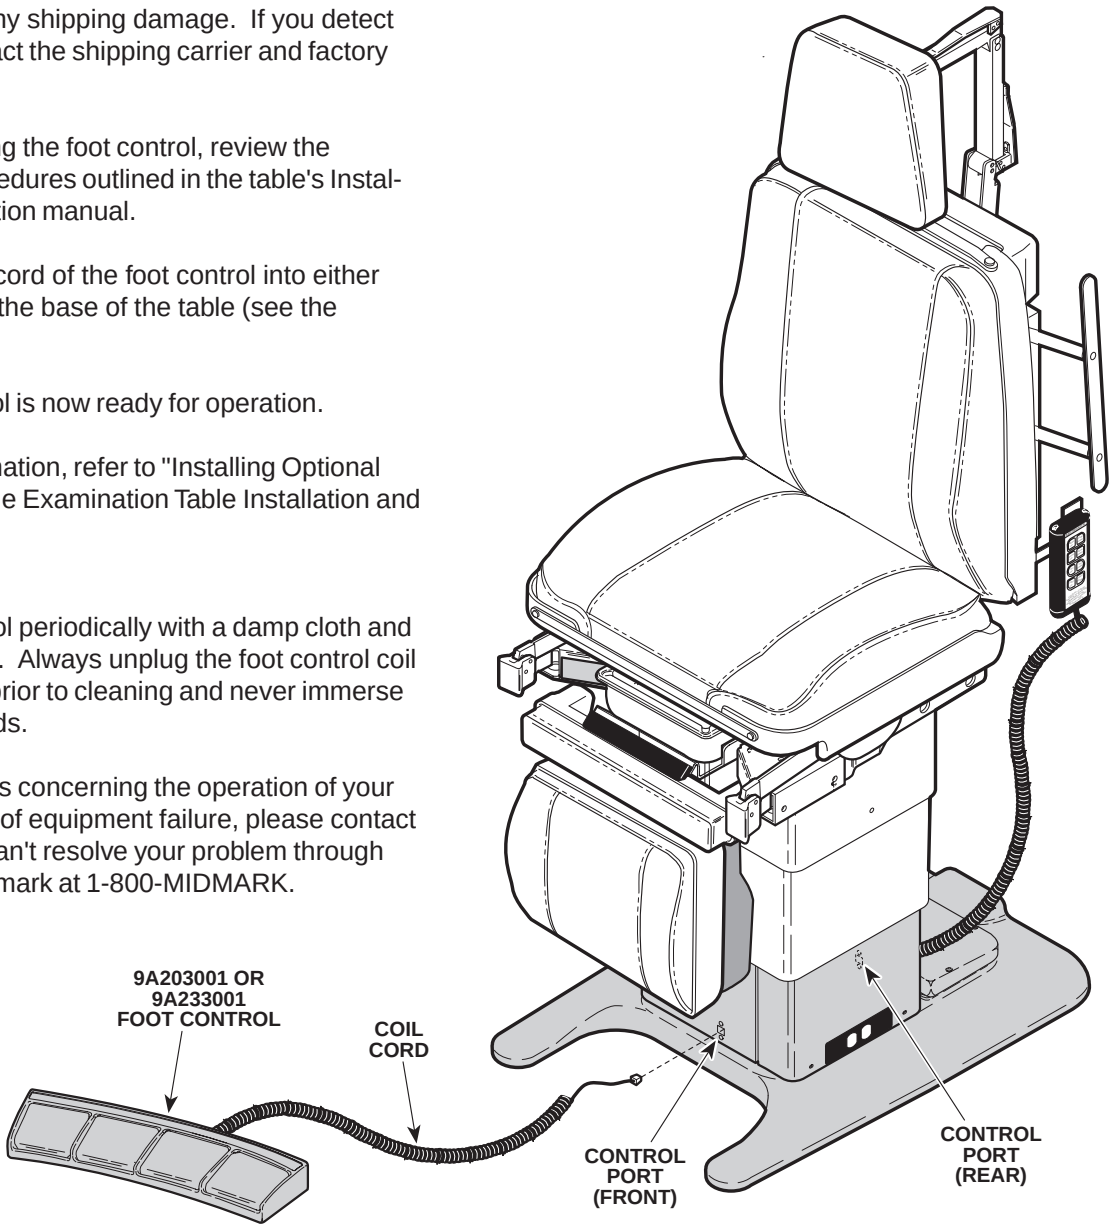

MA281000

FOOT CONTROL INSTALLATION

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
937-526-3662 TELEX 288007 FAX 937-526-5542

© Midmark Corporation - 1995